PANDA BOX™

Cellulite Cavitation

USER MANUAL

CE

ISO13485 Class

PREFACE

Congratulations on your purchase!

You have purchased equipment with the latest technology.We will make the greatest effort to guarantee optimal use of your Device.By following this guide, you can understand easily and quickly how to use all the features of your PANDA BOX.

Thank you thoroughly read the manual before using the device. Carry it always at hand to consult for the best use of your PANDA BOX,If an abnormal situation should happen when using the device, thank you to contact our customer service to our company take steps to rectify the situation promptly.

Cavitation

This section provides safety information critical to use of Diathermy Systems.Read,understand and follow all of the Safety precautions found in this section and throughout this manual prior to system use. Stay current with the latest clinical developments in the fields of CAV Therapy.Observe all applicable precautionary measures for treatment. Keep informed on appropriate indications and contraindi cation for the use of CAV Therapy.

5minutes mix the oil and water

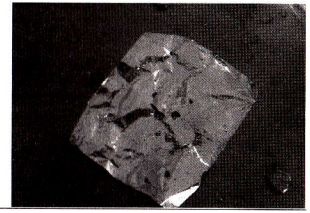

1minutes breakdown the ALU paper

Question about panda box-CAV

What areas can be treated with CAV systems?
Belly,waist,thigh,calf,buttocks.

What areas forbid treated with CAV systems?
The CAV is a deep model ultrasonic,fobid use around eyes and heart.

What do CAV treatments feel like?
When CAV 40K work,can hear zizizi voice like hexapod sound.body can feel warm.Sometimes with the tinnitus.

How many treatments will I need?
4times in frist two weeks,after 1time per week,until satisfying effect.

Warranty

This product is warranted against defects in materals and workmanship for a period of one year from date of shipment.The company will at its option,repair or replace components which prove to be defective during the warranty period,provided that the repairs or replacements are carried out by the company or its approved agents.

The company will consider itself responsible for the effects on safety, eliability and performance of the product.Only if the product is used in accordance with the instructions for use,only if the electrical installation of the relevant room complies with the appropriate national requirements. Should the product be returned to the company for repair it must be sent carriage paid.Consumable items,for example,Probe and Display Are not excluded from the above warranty.

CAUTION

• Read,understand and practice all precautionary and operating instructions.Know the limitations and hazards associated with using any electrical stimulation,ultrasound device or any other device.

• DO NOT operate the unit in an environment of short-wave diathermy use.

• The Lower frequency generator should be routinely checked before each use to determine that all controls function

• normally,especially that the intensity control does properly adjust the intensity of the power output in a stable manner.Also,determine that the treatment time control does actually terminate power output when the timer reaches zero.

• DO NOT use sharp objects such as a pencil point or ballpoint pen to operate the buttons on the control panel as damage may result.

• This system,optional modules and associated accessories should be operated,transported and stored in temperatures between -20to35 degree,with relative humidity ranging from 30%-60%.

• Electrodes with care,inappropriate handing of the applicator may adversely affects characteristics.

• Before each use inspect applicator for cracks,which may allow the ingress of conductive fluid.

• Inspect electrode,cables and associated connectors before each use.

• The PANDA BOX-CAV,optional modules and some associated accessories are not designed to prevent the ingress of water or liquids.Ingress of water or liquids could cause malfunction of internal components of the system and therefore create a risk of injury to the patient.

WARNING

• This device should be used in clinic or home.

• Make certain the unit is electrically grounded by connecting only to a grounded electrical service receptade conforming to the applicable national and local electrical codes.

• This device should be kept away from children.

• Care must be taken when operating this equipment around other equipment.
Potential electromagnetic or other interference could occur to this or to the other equipment.Tyr to minimize this interference by not using other equipment in conjunction with it.

• Use of controls or adjustments or performance of procedures other than those sepecified herein may result in hazardous conditions causing damage to the system,optional modules,associated accessories and hazardous exposure to energy.

• To prevent electrical shock,disconnect the unit from the power source (electrical outlet) before attempting any maintenance procedures to the system.

• Do not use cracked electrode when it have any crack on the surface.

Parameter

- Working Freqency:40Khz
- Energy:1-3W/cm2 adjust
- Active Surface:12cm2
- Pulse Type:continuous
- Voltage:110/220v
- Size:37x33x21cm
- Weight:1.5kg

Application

- Intensive physical lipolysis to remove surplus fat
- Burn surplus fat, Lymphatic Treatment
- skin tightening, improve skin elasticity
- Improve orange peel organization, body shaping

Operate Panel

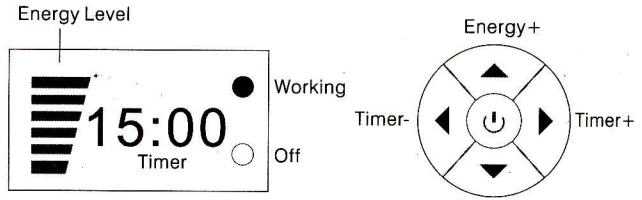

After turn on power,Adjust the energy and time,then press ⏻ the device Working,then press again ⏻ the machine stop.
The system default:5minutes/3Energy Level
The Sytem Max Energy:6Level,Max Timer:15Minutes

PANDA BOX-RF Diagram Reference

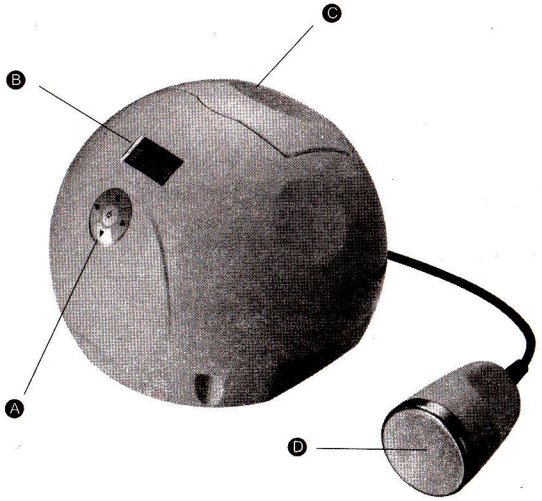

A.Control Panel
B.Display
C.Handle holder
D.Probe
E.Power switch
F.Power Plug





Familiarize yourself with the features

- During the treatment,Must put the GEL on skin.
- Do not let the machine working more than 1hours continuous.
- After finish the treatment,need clean the probe.
- For any hypersensitive skin,need use lower level energy to make test.
- Do not put the probe in Metal Ground.

Pre-startup preparations

1.Upacking and Inspection
After unpacking, please check to ensure that the instrument is not seriously damaged,circuit lines are
well connected and accessories are available (see accessories list)Must connect well the handle socket.

2.Checking power voltage
Ensure that the power voltage complies with the requirement of the instrument.

3.Connecting power cable
(Make sure the ground socket is in working order.)

Operation procedures

1.Operateion prelude
Let the treatment probe touch the target area
and mover(Or Slide)from the inner to the outer and round and round and from the lower place to the higher,do it as this way time by time.when you do the treatment on the upper lid,Pls move a bit more quickly,when the gel on the skin get drier,please add some GEL and go on with the treatment.
the ultrasonic GEL thickness is around 3-5mm.

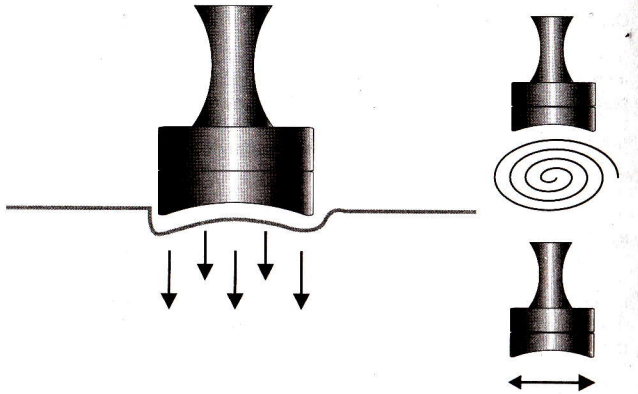

2.Treament process
a.Drink some water
b.clean skin
c.massage with body slimming distillate
d.Smear body slimming diatillate on skin and apply treatment with probe.
e.clean skin
f.put the GEL on skin.
g.put the probe on skin for treatment.

Course of treatment:4times in frist 2weeks,after that 1time treament per Week.10times per course.
After frist one or two treatment,the Cellulite will lost 2-3kg.the Waist will lost 2-4cm.The skin will become lift.
After one course of treatment;Skin becomes compact and flabby skin is improved.The Cellulite will lost 5-10kg

3.treatment Caution

3.1.for treatment is that the patient should feel hot but not very or burned.

3.2.Keep the skin be wet,put more gel or spray more water.

3.3.patient must drink some water during treatment.

3.4.Do not apply on areas such as around the eyes and heart.

Contraindication

- To avoid using the machine on the abdomen of the pregnant women or women in menses
- To avoid using the machine on around the parts under which metal or any conductor.
- To avoid using the machine on the epileptic and those in bad health
- To avoid using the machine on the wound around the treatment area and the areas with metals inside of the body.
- To avoid using the machine on those with over expert on the result.
- To avoid using the machine on people who has high blood pressure or diabetes or serious skin diseases or heart diseases,or who is sensitive to electric current,or who is reveiving hormone treatment.